

# Appendix D

## Performance Specifications

### SYSTEM PERFORMANCE

#### Frequency Range:

#### RF Models:

37317A 22.5 MHz to 8.6 GHz

#### Microwave Models

37325A 40 MHz to 13.5 GHz

37347A 40 MHz to 20 GHz

37369A 40 MHz to 40 GHz

37397A 40 MHz to 65 GHz

#### Dynamic Range:

The following table gives dynamic range in two manners. "Receiver Dynamic Range" is defined as the ratio of the maximum signal level at Port 2 for 0.1 dB compression to the noise floor at Port 2.

Model	Freq (GHz)	Max Signal Into Port 2 (dBm)	Noise Floor (dBm)	Receiver Dynamic Range	Port 1 Power (dBm)	System Dynamic Range
37317A	0.0225	+30	-95	125	0	95
	2	+30	-98	130	0	98
	8.6	+30	-98	130	0	98
37325A	0.04	+30	-65	100	+5	70
	2	+30	-93	128	+5	98
	13.5	+30	-93	128	+5	98
37347A	0.04	+30	-65	100	+5	70
	2	+30	-93	128	+5	98
	20	+30	-91	126	+5	96
37369A	0.04	+30	-65	100	+5	58
	2	+30	-93	128	+5	86
	20	+30	-90	125	0	83
	40	+30	-83	123	-7	76
37397A	0.04	+30	-77	107	+10	70
	2	+30	-105	135	+10	98
	20	+30	-97	127	-2	90
	40	+30	-95	125	-7	88
	50	+30	-87	117	-2	80
	65	+30	-77	107	-2	70

"System Dynamic Range" is defined as the ratio of the power incident on Port 2 in a through line connection to the noise floor at Port 2 (forward measurements only). In preparing the table, 10 Hz IF bandwidth and 512 averages were used in calibration and measurement.

#### High Level Noise (typical)

<0.04 dB and <0.5° peak-to-peak variation in a 1 kHz IF bandwidth up to 20 GHz. <0.08 dB and <1.0° peak-to-peak variation up to 40 GHz. <0.25 dB and <2.5° peak-to-peak variation up to 65 GHz.

#### Measurement Throughput:

Measurement times are based on a single 40 MHz to 20 GHz sweep with 10 kHz IF bandwidth (no averages) after a full 12-term calibration. Sweep times include retrace and bandswitch times.

#### Measurement Time (ms) vs. Data Points (typical):

Calibration Type	Data Points				
	3	51	101	401	1601
1 Port (3 Term)	60	250	330	960	3300
Full 2 Port	60	270	400	1000	3600

#### Measurement Time vs. Sweep Mode for 101 Data Points (typical):

Sweep Mode	Time (ms)
Linear	350
List	350
CW	230

#### Measurement Time vs. IF Bandwidth for 101 Data Points (typical):

IF Bandwidth	Time (ms)
10 kHz	350
1 kHz	530
100 Hz	1900
10 Hz	14000

Connector	Frequency (GHz)	Directivity (dB)	Source Match (dB)	Load Match (dB)	Reflection Frequency Tracking (dB)	Transmission Frequency Tracking (dB)	Isolation (dB)
GPC-7	0.0225	>52	>44	>52	±0.003	±0.004	>105
	2.0	>52	>44	>52	±0.003	±0.004	>115
	18	>52	>42	>52	±0.004	±0.012	>112
GPC-7 LRL Calibration	2.0	>60	>60	>60	±0.001	±0.001	>115
	18	>60	>60	>60	±0.001	±0.001	>112
N-Type	0.0225	>46	>36	>46	±0.004	±0.004	>105
	2.0	>44	>36	>44	±0.004	±0.004	>115
	18	>40	>32	>40	±0.005	±0.012	>112
3.5 mm	0.0225	>44	>40	>44	±0.005	±0.030	>105
	2.0	>44	>40	>44	±0.005	±0.030	>115
	20	>44	>38	>44	±0.006	±0.050	>110
	26.5	>44	>34	>44	±0.006	±0.070	>102
K	0.0225	>42	>40	>42	±0.005	±0.030	>105
	2.0	>42	>40	>42	±0.005	±0.050	>115
	20	>42	>34	>42	±0.006	±0.070	>110
	40	>38	>34	>38	±0.006	±0.080	>100
V	0.04	>70	>36	>40	±0.050	±0.030	>105
	2.0	>40	>36	>40	±0.050	±0.050	>115
	20	>40	>36	>40	±0.060	±0.070	>110
	40	>36	>32	>36	±0.060	±0.080	>100
	50	>34	>30	>34	±0.080	±0.100	>90
	65	>34	>28	>34	±0.100	±0.120	>80

**Measurement Time vs. Span for 101 Data Points (typical):**

Frequency Span	Time (ms)
40 MHz to 40 GHz	500
20 GHz to 40 GHz	400
10 GHz to 11 GHz	250

**TEST PORT CHARACTERISTICS**

The specifications in the following table apply when the proper Model 34U Universal Test Port Adapters are connected, with or without phase equal insertables, to the test set ports and calibrated with the appropriate Anritsu or other designated calibration kit at 23°C ±3°C using the OSL calibration method with a sliding load to achieve 12-Term error correction (A 90 minute warm-up time is recommended.)

**MEASUREMENT CAPABILITIES**

**Number of Channels:** Four independent measurement channels.

**Parameters:** S11, S21, S22, S12, or user-defined combinations of a1, a2, b1, and b2. All measurements are made without the need to manually reverse the test device.

**Measurement Frequency Range:** Frequency range of measurement can be narrowed within the calibration range without recalibration. CW mode permits single frequency measurements, also without recalibration. In addition, the

system accepts N discrete frequency points where  $2 \leq N \leq 1601$ .

**Domains:** Frequency Domain, CW Draw, and optional High Speed Time (Distance) Domain.

**Formats:** Log Magnitude, Phase, Log Magnitude and Phase, Smith Chart (impedance), Smith Chart (Admittance), Linear Polar, Log Polar, Group Delay, Linear Magnitude, Linear Magnitude and Phase, Real, Imaginary, Real and Imaginary, SWR, Power.

**Data Points:** 1601 maximum. Data points can be switched to a value of 801, 401, 201, 101, or 51 points without recalibration (if 1601 points were used in the calibration). In addition, the system accepts an arbitrary set of N discrete data points where:  $2 \leq N \leq 1601$ . CW mode permits selection of a single data point without recalibration.

**Reference Delay:** Can be entered in time or in distance (when the dielectric constant is entered). Automatic reference delay feature adds the correct electrical length compensation at the push of a button. Software compensation for the electrical length difference between reference and test is always accurate and stable since measurement frequencies are always synthesized. In addition, the system compensates reference phase delay for dispersive transmission media, such as waveguide and microstrip.

**Markers:** Six independent markers can be used to read out measurement data. In delta-reference marker mode, any one marker can be selected as the reference for the

other five. Markers can be directed automatically to the minimum or maximum of a data trace.

**Enhanced Markers:** Marker search for a level or bandwidth, displaying an active marker for each channel, and discrete or continuous (interpolated) markers.

**Marker Sweep:** Sweeps upward in frequency between any two markers. Recalibration is not required during the marker sweep.

**Limit Lines:** Either single or segmented limit lines can be displayed. Two limit lines are available for each trace.

**Single Limit Readouts:** Interpolation algorithm determines the exact intersection frequencies of test data and limit lines.

**Segmented Limit Lines:** A total of 20 segments (10 upper and 10 lower) can be generated per data trace. Complete segmented traces can be offset in both frequency and amplitude.

**Test Limits:** Both single and segmented limits can be used for PASS/FAIL testing. The active channel's PASS or FAIL status is indicated on CRT after each sweep. In addition, PASS/FAIL status is output through the rear panel I/O connector as selectable TTL levels (PASS=0V, FAIL=+5V, or PASS=+5V, FAIL=0V).

**Tune Mode:** Tune Mode optimizes sweep speed in tuning applications by updating forward S-parameters more frequently than reverse ones. This mode allows the user to select the ratio of forward sweeps to reverse sweeps after a full 12-term calibration. The ratio of forward sweeps to reverse sweeps can be set anywhere between 1:1 to 10,000:1.

#### DISPLAY CAPABILITIES

**Display Channels:** Four, each of which can display any S-parameter or user defined parameter in any format with up to two traces per channel for a maximum of eight traces simultaneously. A single channel, two channels (1 and 3, or 2 and 4), or all four channels can be displayed simultaneously. Channels 1 and 3, or channels 2 and 4 can be overlaid.

**LCD:** Color, 8.5-inch diagonal.

**Trace Color:** The color of display traces, memory, text, markers and limit lines are all user definable.

**Trace Overlay:** Displays two data traces on the active channel's graticule simultaneously. The overlaid trace is displayed in yellow and the primary trace is displayed in red.

**Trace Memory:** A separate memory for each channel can be used to store measurement data for later display or subtraction, addition, multiplication or division with current measurement data.

#### Scale Resolution (minimum):

**Log Magnitude:** 0.001 dB/div

**Linear Magnitude:** 1 pU

**Phase:** 0.01°

**Group Delay:** 0.001 ps

**Time:** 0.001 ms

**Distance:** 0.1  $\mu$ m

**SWR:** 1 pU

**Power:** 0.05 dB

**Autoscale:** Automatically sets Resolution and Offset to fully display measurement data.

**Reference Position:** Can be set at any graticule line.

**Annotation:** Type of measurement, vertical and horizontal scale resolution, start/stop or center/span frequencies, and reference position.

**Blank Frequency Information:** Blanking function removes all references to displayed frequencies on the CRT. Frequency blanking can only be restored through a system reset or GPIB command.

#### MEASUREMENT ENHANCEMENT

**Data Averaging:** Averaging of 1 to 4096 averages can be selected. Averaging can be toggled on/off with front panel button. A front panel button turns data averaging on/off, and a front panel LED indicates when averaging is active.

**Video IF Bandwidth:** Front panel button selects four levels of video IF bandwidth. MAXIMUM (10 kHz), NORMAL (1 kHz), REDUCED (100 Hz) and MINIMUM (10 Hz).

**Trace Smoothing:** Functions similarly to Data Averaging but computes an average over a percentage range of the data trace. The percentage of trace to be smoothed can be selected from 0 to 20% of trace. Front panel button turns smoothing on/off, and front panel LED indicates when smoothing is active.

#### SOURCE CONTROL

**Frequency Resolution:** 1 kHz (1 Hz standard on RF units and optional on Microwave units - Option 10A)

**Source Power Level:** The source power (dBm) may be set from the 373XXA front panel menu or via GPIB. Refer to Level Control Range table on next page.


In addition, the port 1 power may be attenuated in 10 dB steps, using the internal 70 dB (60 dB for 37397A) step attenuator. Similarly, high input signals into port 2, not exceeding 1 watt, can be attenuated up to 40 dB, using the internal port 2 step attenuator.

**Power Accuracy:**  $\pm 0.5$  dB at 2 GHz at default power.

**Power Meter Correction:** The 373XXA offers a user-selectable feature that corrects for test port power variations and slope (on Port 1) using an external Hewlett-Packard 437B or Anritsu ML8403 power meter. Power meter correction is available at a user-selectable power level, if it is within the power adjustment range of the internal source. Once the test port power has been flattened, its level may be changed within the remaining power adjustment range of the signal source.


**Set-On Receiver Mode:** The 373XXA can be configured to measure the relative harmonic level of test devices with Set-On Receiver Mode capability. The 373XXA's unique

LOG MAG Ref= 0dBm 5dB/DIV

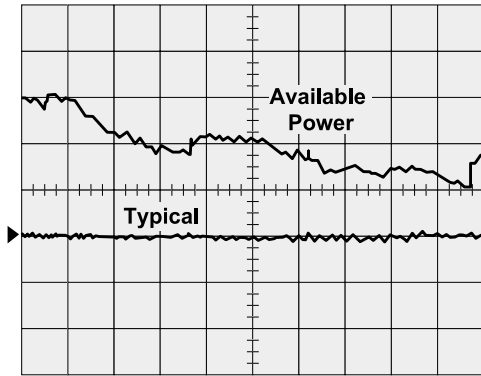


22.5 MHz 8.6 GHz  
Model 37317A Port 1 Power

LOG MAG Ref= -7dBm 5dB/DIV

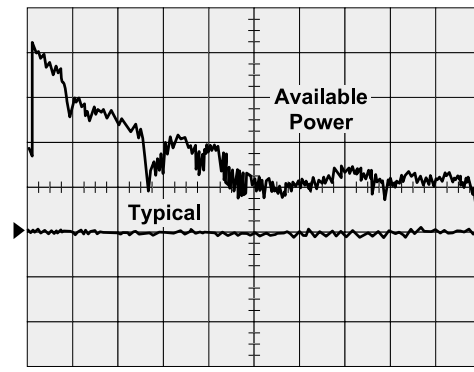


40 MHz 65 GHz  
Model 37397A Port 1 Power

LOG MAG Ref= -7dBm 5dB/DIV

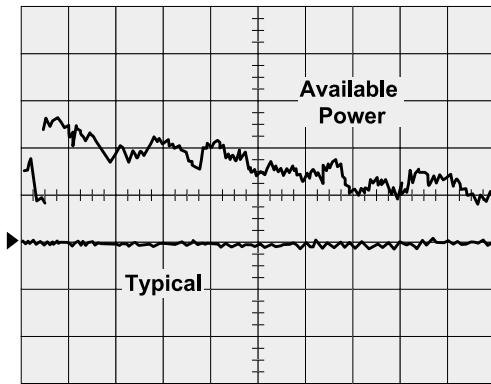

40 MHz 20 GHz  
Model 37325A and 37347A Port 1 Power

LOG MAG Ref= -7 dBm 5dB/DIV

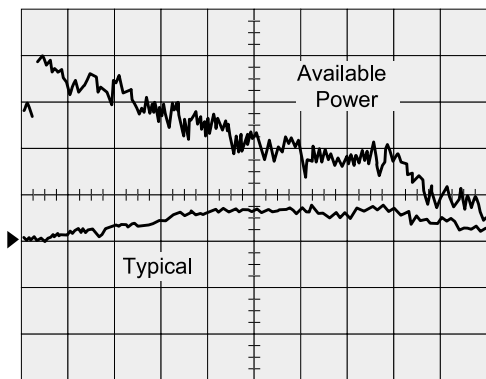

40 MHz 40 GHz  
Model 37369A Port 1 Power

phase locking scheme allows it to operate as a tuned receiver by locking all of its local oscillators to its internal crystal reference oscillator. Set-On Receiver Mode capability significantly increases the versatility of the 373XXA VNA in applications that check for harmonics, intermodulation products, and signals of known frequency.

**Dual Source Control Capability:** Dual Source Control capability allows a user to independently control the frequencies of two sources and the receiver without the need for an external controller. The frequency ranges and output powers of the two sources may be specified. A frequency sweep may be comprised of up to five separate bands, each with independent source and receiver settings, for convenient testing of frequency translation devices such as mixers. Up to five sub-bands may be tested in one sweep. This feature enables users to easily test mixers, up/down converters, multipliers, and other frequency conversion devices.

**Source 1:** The 373XXA internal source or any of the family of 68XXXB, 69XXXA, or 6700B synthesizers..

**Source #2:** Any of ANRITSU's family of 68XXXB, 69XXXA, or 6700B synthesizers.

**Sweep Type:** Linear, CW, Marker, or N-Discrete point sweep.

**POWER RANGE**

Model	Rated Power (dbm)	Minimum Power (dBm)	Resolution (dB)
37317A	0	-95	0.05
37325A	+5	-90	0.05
37347A	+5	-90	0.05
37369A	-7	-97	0.05
37397A	-7	-79	0.05

**LEVEL CONTROL RANGE**  
(Without step attenuator)

	37317A	37325A	37347A	37369A	37397A
Above Reset Power*	+10 dB	+10 dB	+10 dB	+20 dB	+20 dB
Below Reset Power	-25 dB	-25 dB	-25 dB	-20 dB	-20 dB <47 GHz -12 dB ≥47 GHz

\*Source power above the reset level is allowed but not guaranteed, especially over the full frequency range.

**POWER FLATNESS**

Frequency Range (GHz)	Flatness (dB)
0.0225 to 13.5	±1.5
13.5 to 20	±2.0
20 to 40	±3.0
40 to 65	±5.0

**SOURCE PURITY**

(Specifications apply for all models at maximum rated power.)

**Harmonics & Harmonic Related:**

15 dBc (37325A, 37347A, 37369A, 37397A)

35 dBc (37317A)

**Nonharmonics:** 35 dBc (standard)

**Phase Noise:** >60 dBc/Hz at 10 kHz offset and 20 GHz center frequency

**SOURCE FREQUENCY ACCURACY**

**Standard Time Base:**

**Aging:** <1 x 10<sup>-6</sup>/year

**Stability:** <1 x 10<sup>-6</sup> over +15°C to +50°C range

**High Stability Time Base (Option 10):**

**Aging:** <1 x 10<sup>-9</sup>/day

**Stability:** <5 x 10<sup>-9</sup> over 0°C to +55°C range

**GROUP DELAY CHARACTERISTICS**

Group Delay is measured by computing the phase change in degrees across a frequency step by applying the formula:

$$\tau_g = -1/360 \frac{d\Phi}{df}$$

**Aperture:** Defined as the frequency span over which the phase change is computed at a given frequency point. The aperture can be changed without recalibration. The minimum aperture is the frequency range divided by the number of points in calibration and can be increased to 20% of the frequency range without recalibration. The frequency width of the aperture and the percent of the frequency range are displayed automatically.

**Range:** The maximum delay range is limited to measuring no more than +180° of phase change within the aper-

ture set by the number of frequency points. A frequency step size of 100 kHz corresponds to 10 ms.

**Measurement Repeatability (sweep to sweep):** For continuous measurement of a through connection, RSS fluctuations due to phase and FM noise are:

$$\frac{141 [ (Phase\ Noise\ in\ deg)^2 + (\tau_g \times Residual\ FM\ Noise\ in\ Hz)^2 ]^{0.5}}{360 (Aperture\ in\ Hz)}$$

**Accuracy:**

$$Error\ in\ \tau_g = \frac{\sqrt{Error\ in\ Phase\ (deg)^2}}{360} + [\tau_g \times Aperture\ Freq.\ Error\ (Hz)] / Aperture\ (Hz)$$

**VECTOR ERROR CORRECTION**

There are five methods of calibration:

**1) Open-Short-Load (OSL).** This calibration method uses short circuits, open circuits, and terminations (fixed or sliding)

**2) Offset-Short (waveguide):** This calibration method uses short circuits and terminations.

**3) LRL/LRM:** The Line-Reflect-Line (LRL) or Line-Reflect-Match (LRM) calibration uses transmission lines and a reflective device or termination (LRM).

**4) TRM:** The Thru-Reflect-Match calibration uses short circuits and fixed termination.

**5) AutoCal:** The VNA will serially drive an external AutoCal module to perform a 2-port OSLT calibration. AutoCal is a single two port calibration module with built-in, switched, and characterized OSLT standards. AutoCal provides quick, reliable, and accurate calibrations that exceed the performance of a standard broadband load OSLT calibration.

There are four vector error correction models available:

**1) Full 12-Term**

**2) One Path/Two Port**

**3) Frequency Response (Transmission/Reflection)**

**4) Reflection Only**

Full 12-term can always be used, if desired, since all 373XXA-series models automatically reverse the test signal. Front-panel display indicates the type of calibration stored in memory. Front-panel button selects whether calibration is to be applied, and an LED lights when error correction is being applied.

**Calibration Sequence:** Prompts the user to connect the appropriate calibration standard to Port 1 and/or Port 2. Calibration standards may be measured simultaneously or one at a time.

**Calibration Standards:** For coaxial calibrations the user selects SMA, GPC-3.5, GPC-7, Type N, 2.4 mm, TNC, K, or V Connector from a calibration menu. Use of fixed or sliding loads can be selected for each connector type. User defined calibration standards allow for entry of open

capacitance, load and short inductances, load impedance, and reflection standard offset lengths.

**Reference Impedance:** Modify the reference impedance of the measurement to other than 50 ohms (but not 0).

**LRL/LRM Calibration Capability:** The LRL calibration technique uses the characteristic impedance of a length of transmission line as the calibration standard. A full LRL calibration consists merely of two transmission line measurements, a high reflection measurement, and an isolation measurement. The LRM calibration technique is a variation of the LRL technique that utilizes a precision termination rather than a second length of transmission line. A third optional standard, either Line or Match, may be measured in order to extend the frequency range of the calibration. This extended calibration is achieved by mathematically concatenating either two LRL, two LRM, or one LRL and one LRM calibration(s). Using these techniques, full 12-term error correction can be performed on the 373XXA VNA.

**Adapter Removal Calibration:** Built-in Adapter Removal application software accurately characterizes and "removes" any adapter used during calibration what will not be used for subsequent device measurements. This technique allows for accurate measurement of non-insertable devices.

**Dispersion Compensation:** Selectable as Coaxial (non-dispersive), Waveguide, or Microstrip (dispersive).

**Reference Plane:** Selectable as Middle of line 1 or Ends of line 1.

**Corrected Impedance:** Determined by Calibration Standards.

#### HARD COPY

**Printer:** Menu selects full screen, graphical, tabular data, S2P or Text output, and printer type. The number of data points of tabular data can be selected as well as data at markers only. Compatible with the 2225C InkJet, HP QuietJet, HP 310/320/340 DeskJet, HP 500 Deskjet, HP 560C DeskJet (b/w only), HP LaserJet II, III, & IV Series, and some Epson compatible printers with Parallel (Centronics) interfaces.

**GPIB Plotters:** The 37XXX VNA is compatible with HP Models 7440A, 7470A, 7475A, and 7550A (in standard mode) and Tektronix Model HC100 plotters. Menu selects plotting of full or user-selected portions of graphical data. Plotter is connected to the dedicated GPIB bus.

**Performance:** After selecting the Start Print button, front panel operation and measurement capability is restored to the user within 2 seconds.

#### STORAGE

**Internal Memory:** Ten front panel states (setup/calibration) can be stored and recalled from non-volatile memory locations. The current front panel setup is automatically stored in non-volatile memory at instrument power-down.

When power is applied, the instrument returns to its last front panel setup.

**Internal Hard Disk Drive:** Used to store and recall measurement and calibration data and front-panel setups. All files are MS-DOS compatible. File names can be 1 to 8 characters long, and must begin with a character, not a number. Extensions are automatically assigned.

**External SCSI Interface:** Option 4 deletes the internal hard disk drive, and adds a SCSI Interface connector to the rear panel for connecting a SCSI-2 formatted hard disk drive.

**Internal Floppy Disk Drive:** A 3.5-inch diskette drive with 1.44 Mbytes formatted capacity is used to load measurement programs and to store and recall measurement and calibration data and front panel setups. All files are MS-DOS compatible. File names can be 1 to 8 characters long, and must begin with a character, not a number. Extensions are automatically assigned.

**Measurement Data:** 102.8 kbytes per 1601 point S-parameter data file.

**Calibration Data:** 187.3 kbytes per 1601 point S-parameter data file (12-term cal plus setup).

**Trace Memory File:** 12.8 kbytes per 1601 point channel.

#### GPIB

##### GPIB INTERFACES - 2 PORTS

**System GPIB (IEEE-488.2):** Connects to an external controller for use in remote programming of the network analyzer. Address can be set from the front panel and can range from 1 to 30.

**Interface Function Codes:** SH1, AH1, T6, TE0, L4, LE0, SR1, RL1, PP1, DT1, DC0, C0.

**Dedicated GPIB:** Connects to external peripherals for network analyzer controlled operations (e.g. GPIB plotters, frequency counters, frequency synthesizers, and power meters).

**GPIB Data Transfer Formats:** ASCII, 32-bit floating point, or 64-bit floating point. 32-bit and 64-bit floating point data can be transferred with LSB or MSB first.

##### GPIB DATA COLLECTION SUMMARY

This section summarizes typical data collection times for automated measurements using the 37XXX IEEE 488.2 GPIB bus. Throughput measurements for both tables were made as follows: start the timer, trigger a sweep, wait for a full sweep, transfer data across the GPIB and stop the timer. Data throughput times are shown separately for measurements made without calibration and with full two-port, 12-term calibration.

**Data Transfer Speed (with or without cal):** 150 kbytes/second

**Measurement conditions:** 40 MHz to 20 GHz sweep, single channel, log magnitude display, 10 kHz IF bandwidth, and output final data.

**Throughput Times (ms) without Correction (typical)**

Data Format	3 Points*	101 Points	401 Points	1601 Points
32 Bit	230	650	1400	3600
64 Bit	230	680	1450	4000
ASCII	235	800	1700	5000

**Throughput Times (ms) with Correction (typical)**

Data Format	3 Points*	101 Points	401 Points	1601 Points
32 Bit	340	1200	2600	7800
64 Bit	350	1200	2700	8300
ASCII	350	1280	3000	9300

\* Frequencies taken at 2, 4, and 6 GHz

**GENERAL**

**37300A Front Panel Connectors and Controls:**

**Keyboard Input:** An IBM-AT compatible keyboard can be connected to the front panel for navigating through front panel menus and disk directories, annotation of data files and display labels, printing displays and pausing instrument sweeps.

**Test Ports:** Universal/K, male, connectors are standard on all models except for 37397A, which has V Connector test ports as standard. For other configurations check Option 7. For additional configurations check Test Port Converters.

**Bias Inputs:** Port 1 and 2: 0.5 amps maximum through BNC connectors.

**Port 1 Amplifier Loop:** Access to insert an external amplifier, ahead of the port 1 coupler or bridge, to increase port 1 power output, up to +30 dBm (1 watt) maximum.

**37300A Rear Panel Connectors and Controls:**

**PRINTER OUT:** Centronics interface for an external printer.

**VGA OUT:** Provides VGA output of 373XXA video display.

**10 MHz REF IN:** Connects to external reference frequency standard, 10 MHz, +5 to -5 dBm, 50 ohms, BNC female.

**10 MHz REF OUT:** Connects to internal reference frequency standard, 10 MHz, 0 dBm, 50 ohms, BNC female.

**EXT ANALOG OUT:** -10V to +10V with 5 mV resolution, varying in proportion to user-selected data (e.g., frequency, amplitude). BNC female.

**EXT ANALOG IN:** ±50 volt input for displaying external signals on the CRT in Diagnostics mode. BNC female.

**LINE SELECTION:** Power supply automatically senses 100V, 120V, 220V or 240V lines.

**EXTERNAL TRIGGER:** External triggering for 373XXA measurement, ±1V trigger. 10 kohm input impedance. BNC female.

**REFERENCE EXTENSION:** Provides access to a1 and b1 samplers; K or V Connector, female.

**EXTERNAL SCSI:** Provides SCSI-2 connector for connection of an external SCSI hard disk drive (Opt. 4).

**EXTERNAL I/O:** 25-pin DSUB connector.

**EXTERNAL SCSI:** Provides SCSI-2 connector for connection of an external SCSI hard disk drive (Opt. 4).

**SERIAL:** Provides control for AutoCal module.

**LIMITS PASS/FAIL:** Selectable TTL levels (Pass=0V, Fail=+5V or Pass=+5V, Fail=0V. Additionally, 0 volts (all displayed channels pass) or +5V (any one of 4 displayed channels fail) output pass/fail status (1 line).

**EXTERNAL TRIGGER:** External triggering for 373XXA measurement, ±1V trigger. 10 kohm input impedance. BNC female.

**EXT ANALOG OUT:** -10V to +10V with 5 mV resolution, varying in proportion to user-selected data (e.g., frequency, amplitude). BNC female.

**Power Requirements:** 85-240V, 48-63 Hz, 540 VA maximum

**Dimensions:** 267H x 432W x 585D mm (10.5H x 17W x 23D in.)

**Weight:** 34 kg (75 lb) - Maximum amount specified for 2-man lift requirement.

**ENVIRONMENTAL**

**Storage Temperature Range:** -40°C to +75°C

**Operating Temperature Range:** -0°C to +50°C

**Relative Humidity:** 5% to 95% at +40°C

**EMI:** Meets the emissions and immunity requirements of EN55011/1991 Class A/CISPR-11 Class A EN 50082-1/1993

IEC 801-2/1984 (4 kV CD, 8kV AD)

IEC 1000-4-3/1995 (3 V/m, 80-1000 MHz)

IEC 801-4/1988 (500V SL, 1000V PL)

IEC 1000-4-5/1995 (2 kV L-E, 1kV L-L)


**GAIN COMPRESSION MEASUREMENT CAPABILITY**

The 373XXA simplifies amplifier Gain Compression and AM/PM measurements. Once an appropriate power and frequency schedule is selected, a power meter calibration, at a set level, will calibrate the linear VNA receiver channels, to accurately measure power in dBm. The 37300A supports the HP437B, and Giga-tronics 8540B series power meters. To measure power, b2/1, a user defined parameter, is automatically selected.

**Swept Power Gain Compression:** The 373XXA will display traditional Power out vs. Power in or Phase vs. Power in, at one of up to 10 selectable frequencies. A separate screen will easily show Power out and Power in at 1 dB, or selected level Gain Compression, for all entered frequencies. (Check figure below).

**Swept Frequency Gain Compression:** Once Gain is measured at the starting power, the user increments Power in, observing Normalized Gain vs. Frequency. This aids in

analyzing the most critical compression frequencies of a broadband amplifier.

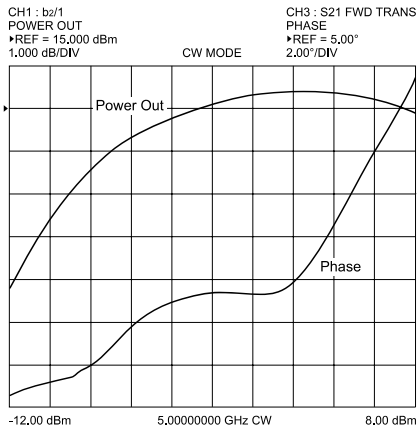

Shows Power Out and Phase performance as a function of Input Power at a CW frequency.

**HIGH SPEED TIME (DISTANCE) DOMAIN MEASUREMENT CAPABILITY (OPTION 2)**

Option 2, High Speed Time (Distance) Domain software allows the conversion of reflection or transmission measurements from the frequency domain to the time domain. Measured S-parameter data is converted to the time domain by application of a Fast Fourier Transform (FFT) using the Chirp Z-Transform technique. Prior to conversion any one of several selectable windowing functions may be applied. Once the data is converted to the time domain, a gating function may be applied to select the data of interest. The processed data may then be displayed in the time domain with display start and stop times selected by the user or in the distance domain with display start and stop distance selected by the user. The data may also be converted back to the frequency domain with a time gate to view the frequency response of the gated data.

**Lowpass Mode:** This mode displays a response equivalent to the classic TDR (Time Domain Reflectometer) response of the device under test. Lowpass response may be displayed in either the impulse or step mode. This type of processing requires a sweep over a harmonic series of frequencies and an extrapolated or user-entered DC value.

**Bandpass Mode:** This mode displays a response equivalent to the time response of the device under test to a band limited impulse. This type of processing may be used with any arbitrary frequency sweep range, limited only by the test set range or device under test response.

**Phasor Impulse Mode:** This mode displays a response similar to the Lowpass impulse response, using data taken over an arbitrary (band limited) sweep range. Detailed information, similar to that contained in the lowpass impulse

response may be used to identify the nature of impedance discontinuities in the device under test. Now, with Phasor Impulse, it is possible to characterize complex impedances on band-limited devices.

**Windowing:** Any one of four window functions may be applied to the initial frequency data, to counteract the effects of processing data with a finite bandwidth. These windows provide a range of tradeoffs of main lobe width versus sidelobe level (ringing).

The general type of function used is the Blackman-Harris window with the number of terms being varied from one to four. Typical performance follows:

Types of Window (Number of Terms)	First Side Lobe Relative to Peak	Impulse Width <sup>1</sup>
Rectangular (1)	-13 dB	1.2W
Nominal-Hamming (2)	-43 dB	1.8W
Low Side Lobe, Blackman-Harris (3)	-67 dB	2.1W
Minimum Side Lobe, Blackman-Harris (4)	-92 dB	2.7W

<sup>1</sup> W(Bin Width) = 1/2Δf sweep width  
 Example: When Δf = 40 MHz to 40 GHz, W = 12.5 ps  
 When Δf = 40 MHz to 65 GHz, W = 7.7 ps

**Gating:** A selective gating function may be applied to the time domain data to remove unwanted responses, either in a pass-band or reject-band (mask). This gating function may be chosen as the convolution of any of the above window types with a rectangular gate of user defined position and width. The gate may be specified by entering start and stop times or center and span. The gated data may be displayed in the time domain, or converted back to the frequency domain.

**Time Domain Display:** Data processed to time domain may be displayed as a function of time or as a function of distance, provided the dielectric constant of the transmission media is entered correctly. In the case of dispersive media such as waveguide or microstrip, the true distance to a discontinuity is displayed in the distance mode. The time display may be set to any arbitrary range by specifying either the start and stop times or the center time and span. The unaliased (non-repeating) time range is given by the formula:

$$UnaliasedRange (ns) = \frac{Number\ of\ Frequency\ Data\ Points}{Frequency\ Sweep\ Range\ (GHz)}$$

The resolution is given by the formula:

$$Main\ Lobe\ Width\ (null\ \backslash\ null)\ in\ ns = \frac{kW}{Freq\ Sweep\ Range\ (GHz)}$$



Where  $kW$  is two times the number of window terms (for example, four for a two-term window)

For a 40 GHz sweep range with 1601 data points, the unaliased range is 40.025 nanoseconds.

For a 65 GHz sweep with 1601 data points, the unaliased range is 24.646 nanoseconds.

**Frequency with Time Gate:** Data that has been converted to time domain and selected by the application of gating function may be converted back to the frequency domain. This allows the display of the frequency response of a single element contained in the device under test. Frequency response accuracy is a function of window and gate type, and gate width. For a full reflection, minimum gate and window accuracy is within 0.2 dB of the ungated response over a 40 GHz range.

#### MEASUREMENT UNCERTAINTY

The graphs on pages D-13 through D-15 give measurement accuracy after 12-term vector error correction. The errors are worst case contributions of residual directivity, load and source match, frequency response, isolation, network analyzer dynamic accuracy, and connector repeatability. In preparing the following graphs, 10 Hz IF bandwidth and averaging of 512 points were used (measured at  $23 \pm 3^\circ \text{C}$ ). Changes in the IF bandwidth or averaging can result in variations at low levels.

#### SYSTEM OPTIONS

**OPTION 1, Rack Mounting:** Rack mount kit containing a set of track slides (90 tilt capability), mounting ears, and front panel handles to let the instrument be mounted in a standard 19-inch equipment rack.

**OPTION 1A, Rack Mounting:** Rack mounting kit containing a set of mounting ears and hardware to permanently mount instrument in a standard 19-inch equipment rack.

**OPTION 2, High Speed Time (Distance) Domain Measurement Capability**

**OPTION 4, External SCSI-2 Hard Disk Drive Compatibility:** Provides SCSI-2 rear panel connector for connection of an external SCSI HDD. Remove internal HDD.

**OPTION 7A/N/NF/S/K, Universal Test Port Configuration Replaces Universal/K Connector (standard) with:**

- 7A - Universal/GPC-7
- 7N - Universal/N, male
- 7NF - Universal/N, female
- 7S - Universal/3.5 mm, male

**OPTION 10A, High Stability Time Base:** Replaces the standard temperature compensated crystal oscillator (with a temperature stability of 1ppm over a 0 to  $55^\circ \text{C}$  range) with an ovenized crystal oscillator (aging stability of  $1 \times 10^{-9}$ /day and temperature stability  $5 \times 10^{-9}$  over 0 to  $55^\circ \text{C}$  range). Adds 1 Hz frequency resolution.

#### UPGRADE OPTIONS\*

**37200A** Upgrade to a higher frequency 37200A.

**37200A** Upgrade to an equivalent or higher frequency 37300A.

**37200B** Upgrade to a higher frequency 37200B.

**37200B** Upgrade to an equivalent or higher frequency 37300A.

**37300A** Upgrade to a higher frequency 37300A.

Please call your Anritsu representatives for pricing and delivery.

#### ON-SITE SUPPORT

**Option ES 31:** 3 year on-site repair.

**Option ES 37:** 3 year on-site verification

**Option ES 38:** 3 year on-site Mil-Std verification

**Option ES 51:** 5 year on-site repair.

**Extended Service Options** Additional, two year and four year return to Anritsu service is available, as an option for 373XXA systems and components. Prices and details are available from your Sales Representative or by contacting the factory.

#### CALIBRATION KITS

##### Standard

**3650 SMA/3.5 mm Calibration Kit**

**Option 1:** Male and Female Sliding Terminations

**3651 GPC-7 Calibration Kit**

**Option 1:** Sliding Terminations

**3652 K Connector Calibration Kit**

**Option 1:** Male and Female Sliding Terminations

**3653 Type N Calibration Kit**

**3654B Type V Calibration Kit;** includes male & female sliding terminations

**Economy (8.6 GHz)**

**3750 SMA Calibration Kit**

**3751 GPC-7 Calibration Kit**

**3753 Type N, 50 W, Calibration Kit**

**3753-75 Type N, 75 W, Calibration Kit**

##### VERIFICATION KITS

**3663 Type N Verifications Kit**

**3666 3.5 mm Verifications Kit**

**3667 GPC-7 Verifications Kit**

**3668 K Connector Verifications Kit**

**3669B V Connector Verifications Kit**

##### SEMI-RIGID TEST PORT CABLES

**3670A50-1,** DC to 18 GHz, GPC-7 connectors, 1 foot long, two required.

**3670A50-2,** DC to 18 GHz, GPC-7 connectors, 2 feet long.

**3670K50-1,** DC to 40 GHz, K connectors, 1 foot long, male/female, two required.

**3670K50-2,** DC to 40 GHz, K connectors, 2 feet long, male/female.

**3670V50-1**, DC to 65 GHz, V connectors, 1 foot long, male/female, two required.

**3670V50-2**, DC to 65 GHz, V connectors, 2 feet long, male/female.

#### **FLEXIBLE TEST PORT CABLES**

**3671A50-1 GPC-7 Flexible Cables**, 25 in. (1 pair).

**3671A50-2 GPC-7 Flexible Cable**, 38 in.

**3671S50-1 3.5mm Flexible Cables**, 25 in. (1 pair), male/male.

**3671S50-2 3.5mm Flexible Cable**, 38 in., male.

**3671K50-1 K Connector Flexible Cables**, 25 in.

(1 pair), male/male.

**3671K50-2 K Connector Flexible Cable**, 38 in., male.

**3671V50-1 Universal Test Port Converter On Each Side**, moving the VNAs V-type test port converter to the end of the cable, 25 in., 2 each.

**3671V50-2 Universal Test Port Converter On Each Side**, moving the VNAs V-type test port converter to the end of the cable, 38 in., 1 each.

**NOTE:** All 3671-Series flexible test port cables mate to the standard 34UK50 Universal K Connector Test Port.

#### **TEST PORT CONVERTERS**

**34UA50 Test Port Converter**, Universal/GPC-7

**34UK50 Test Port Converter**, Universal/K Connector, male

**34UN50 Test Port Converter**, Universal/N, male

**34UNF50 Test Port Converter**, Universal/N, female

**34UQ50 Test Port Converter**, Universal/2.4 mm, male

**34US50 Test Port Converter**, Universal/3.5 mm, male

**01-202**, Wrench, for changing test set Test Port Converters.

#### **GPIB CABLES**

**2100-1 GPIB Cable**, 1 m (3.3 ft.)

**2100-2 GPIB Cable**, 2 m (6.6 ft.)

**2100-4 GPIB Cable**, 4 m (13.2 ft.)

**2100-5 GPIB Cable**, 0.5 m (1.65 ft.)

#### **ACCESSORIES**

**2000-660 HP 310 Deskjet Printer**, Printer Stand, Deskjet Printer Cartridge and Power cord.

**2000-661 Extra Printer Cartridge**

**2000-662 Rechargeable Battery**

**2000-663 Power Cable**, Europe

**2000-664 Power Cable**, Australia

**2000-665 Power Cable**, U.K.


**2000-666 Power Cable**, Japan

**2000-667 Power Cable**, South Africa


**2225-1 Spare Parallel Interface Printer Cable**

Model 37347A (K Connectors)  
 Reflection Measurements:

Reflection Magnitude Uncertainty  
 37x47A/B/3652/Reflection Only

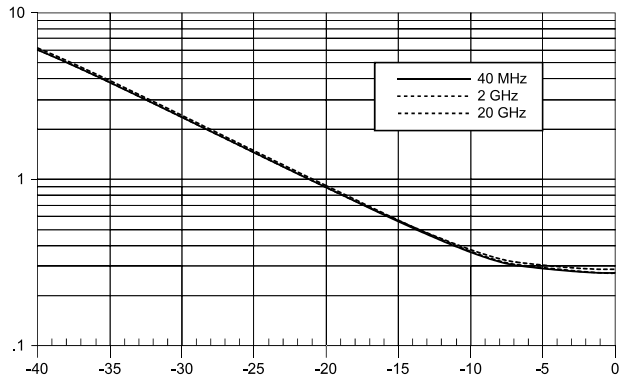


Reflection Phase Uncertainty  
 37x47A/B/3652/Reflection Only

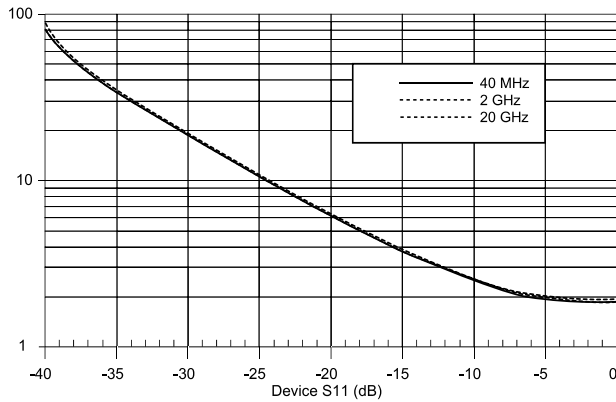


Model 37347A (K Connectors)  
 Transmission Measurements:

Transmission Magnitude Uncertainty  
 37x47A/B/3652/Transmission Only

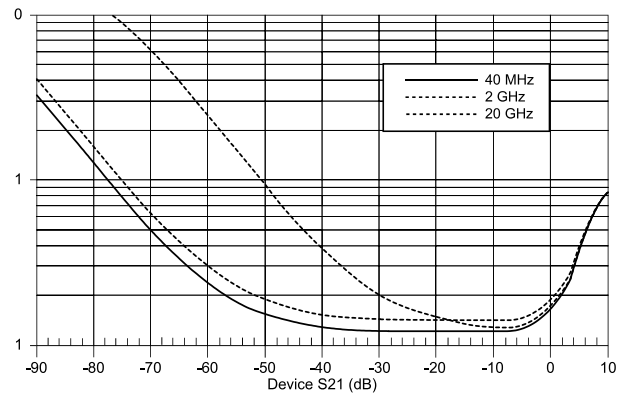


Transmission Phase Uncertainty  
 37x47A/B/3652/Transmission Only

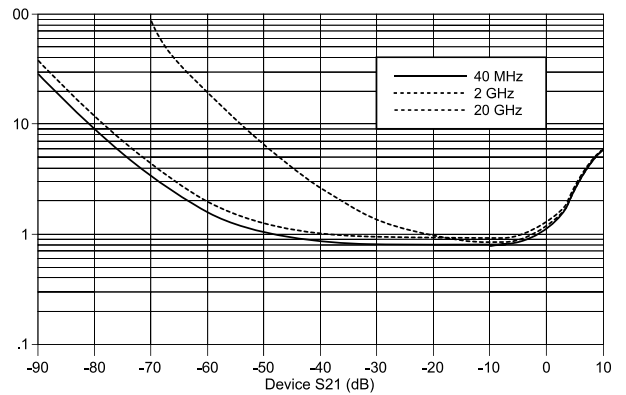


*Model 37369A (K Connectors)*

*Reflection Measurements:*

**Reflection Magnitude Uncertainty**  
37x69A/B/3652/Reflection Only

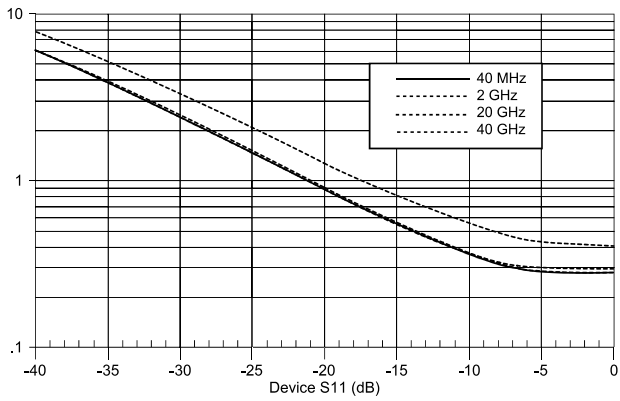


**Reflection Phase Uncertainty**  
37x17A/B/3650/Reflection Only

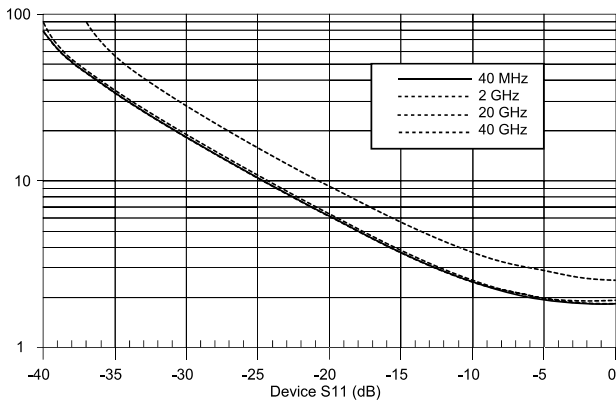


*Model 37369A (K Connectors)*

*Transmission Measurements:*

**Transmission Magnitude Uncertainty**  
37x69A/B/3652/Transmission Only

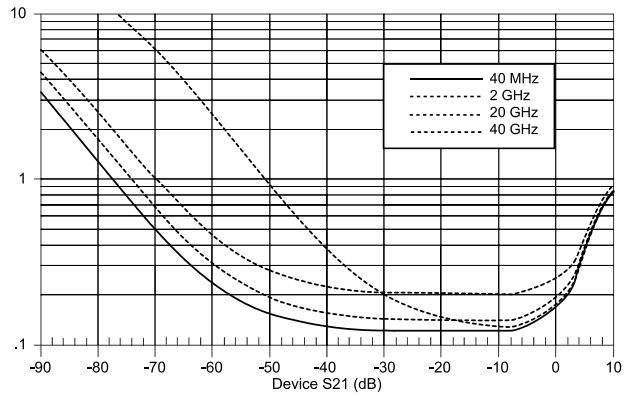


**Transmission Phase Uncertainty**  
37x69A/B/3652/Transmission Only

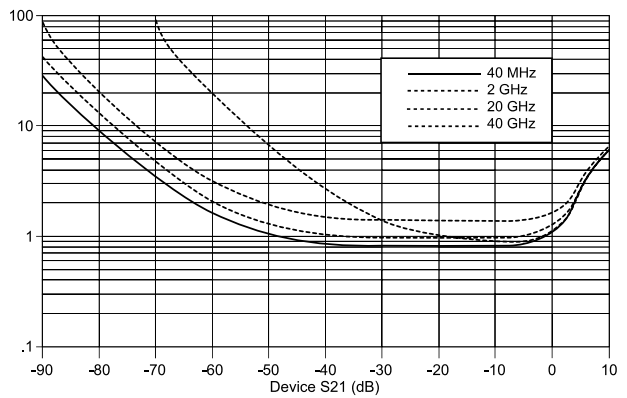


*Model 37397A (V Connectors)*  
*Reflection Measurements:*

**Reflection Magnitude Uncertainty**  
 37x97A/B/3654B/Reflection Only

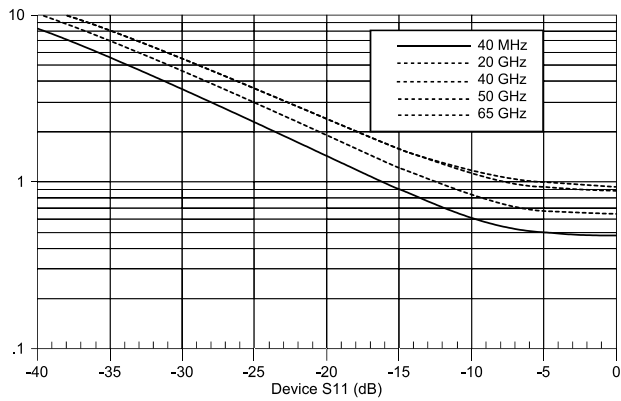


**Reflection Phase Uncertainty**  
 37x97A/B/3654B/Reflection Only

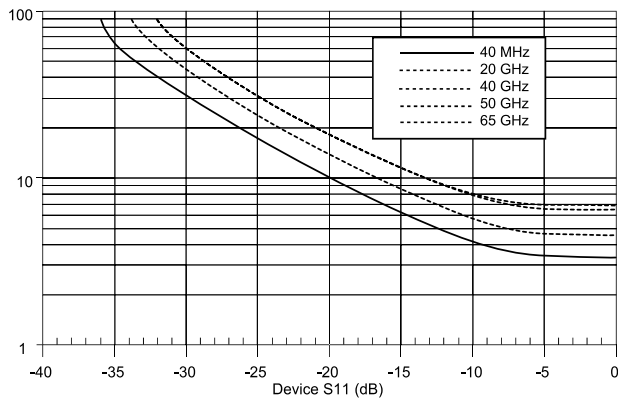

*Model 37397A (V Connectors)*  
*Transmission Measurements:*

**Transmission Magnitude Uncertainty**  
 37x97A/B/3654B/Transmission Only

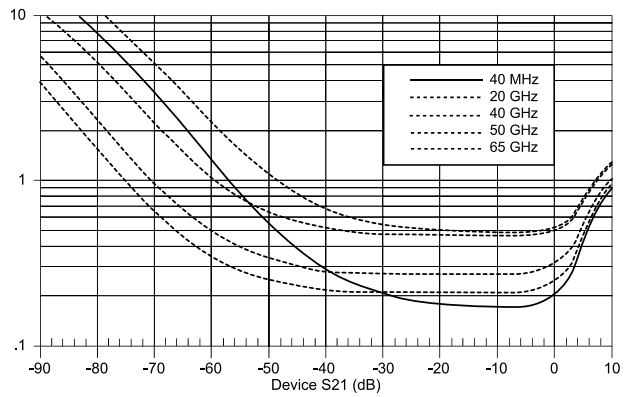

**Transmission Phase Uncertainty**  
 37x97A/B/3654B/Transmission Only

